

# On-line Process Gas Analysis in Ethylene Production Plants

## APPLICATION

Emerson provides Rosemount Analytical gas analyzer technology for on-line analysis in ethylene production plants. Strategically placed gas analyzers improve the process efficiency and the purity of the end product.


## BACKGROUND

Ethylene is one of the most common building blocks in the petrochemical industry with millions of tons produced around the world every year. A typical ethylene plant also produces a number of other important building block chemicals such as propylene and butadiene along with an aromatics-rich pyrolysis gasoline. Ethylene, propylene and butadiene undergo value-added processing in order to synthesize plastics, rubber, fibers and many other organic products.

## GAS ANALYZER APPLICATIONS

Cracked gases such as ethane and propane from petroleum refining overheads and naphtha streams are used as feedstock for ethylene and propylene production. The typical ethylene plant is divided into two basic sections: the cracking furnaces (hot side) and the fractionation train (cold side). The furnaces are often called by different names such as pyrolysis furnaces, naphtha cracking furnaces, naphtha steam crackers, etc. After the cracking furnaces the gases are cooled, compressed and scrubbed. The liquid hydrocarbons and hydrogen are then sent to the fractionation train where they go through several stages of distillation to separate desirable end products and recyclables such as hydrogen, methane, ethylene, ethane, propylene, propane, butylenes, butadiene and gasoline.

## CRACKING FURNACES

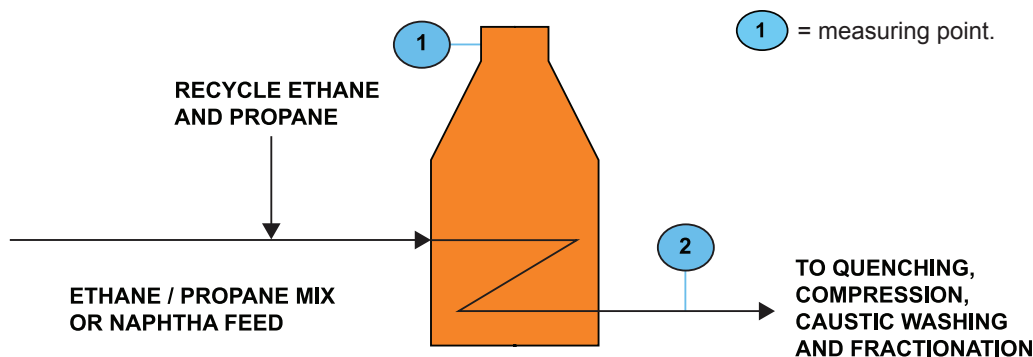

### Measuring Point 1: Combustion in the Cracking Furnaces

Combustion flue gas analyzers placed after each burner ensure optimum fuel/air ratios for combustion efficiency, and also augment the heat balance of the furnace, helping eliminate "hot spots" which promote coking.

The OCX 8800 can be used to provide an oxygen measurement using a zirconium oxide sensor as well as a combustibles measurement. Special accommodations must be made for the high flue gas temperatures just downstream of each burner.

### Measuring Point 2: Decoking of the Cracking Furnaces

After approximately every 20 days of operation, the cracking furnaces need to be decoked since the furnace coils acquire a coating of carbon over time and lose efficiency. This is done by burning off the coke with air in a steam atmosphere. The progress of the decoking phase is monitored by measuring the amount of carbon dioxide in the effluent. It rises as the carbon is burned off and then decreases to zero when the furnaces are clean again and the plant can be returned to normal operation.


Carbon dioxide concentration can be measured using an NDIR (non-dispersive infrared) photometric detector in an X-STREAM analyzer. A specialized probe called a "pyrolysis" or "reflux" probe must first condition it. This probe strips out the tars and other contaminants from the sample before it is sent to the analyzer.

**ROSEMOUNT**  
Analytical

Visit our website at [www.raihome.com](http://www.raihome.com)  
On-line ordering available.

  
**EMERSON**  
Process Management

# FRACTIONATION TRAIN

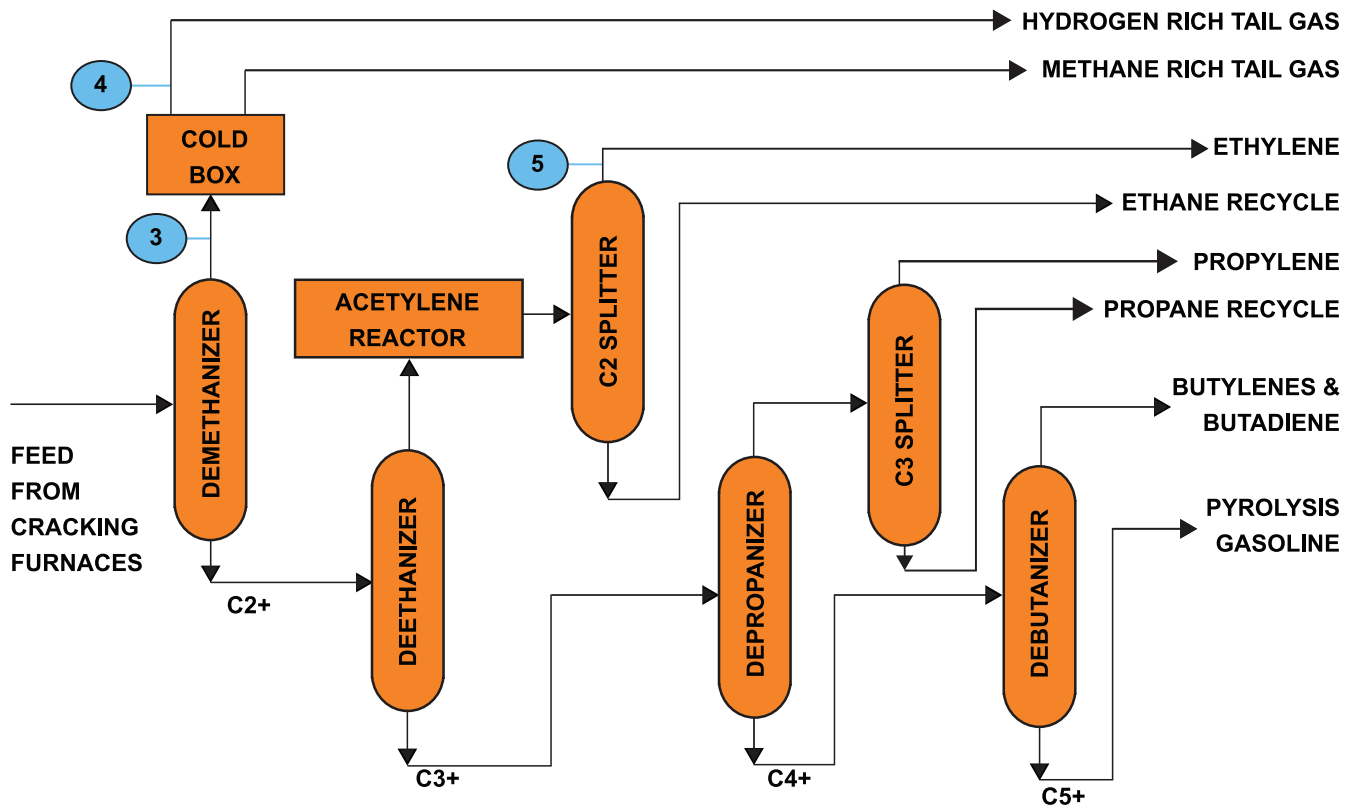

## Measuring Point 3: Ethylene in Demethanizer Overhead

Hydrogen and methane are removed in the first demethanizer for use in the fuel gas header system. A gas analyzer is used to measure ethylene concentration in the demethanizer overhead because loss of valuable ethylene product in the overhead of the demethanizer is undesirable. Operation of the demethanizer is adjusted to minimize the ethylene content in the fuel gas overhead.

## Measuring Point 4: Hydrogen Purity in Demethanizer Overhead after Cold Box

The demethanizer overhead enters a cold box where the stream is further separated into hydrogen rich tail gas and methane rich tail gas. A gas analyzer is used to measure the hydrogen concentration of the hydrogen rich tail gas to confirm that that it is pure enough to be used as needed in the ethylene plant.

## Measuring Point 5: Ethane Impurity in Ethylene in C2 Splitter Overhead

The C2 splitter separates the ethylene product from ethane. The ethane is returned to the furnaces for cracking. A gas analyzer is used to measure ethane concentration in the C2 splitter overhead. Operation of the C2 splitter is adjusted to minimize the ethane impurity in the ethylene product. Sometimes the ethylene product purity is also monitored for residual carbon dioxide traces.

The X-STREAM analyzer is extremely well-suited to make the ethylene, ethane, carbon dioxide and hydrogen measurements described above. The ethylene, ethane and carbon dioxide concentrations are measured using NDIR photometric detectors. The hydrogen concentration is measured using a thermal conductivity detector.

## SUMMARY

Emerson can supply either Rosemount Analytical X-STREAM Flameproof analyzers or X-STREAM Field Housings with purge/pressurization systems for these applications. The analyzers are used to insure more efficient production and higher quality product.

*The contents of this publication are presented for informational purposes only, and while every effort has been made to ensure their accuracy, they are not to be construed as warranties or guarantees, express or implied, regarding the products or services described herein or their use or applicability. All sales are governed by our terms and conditions, which are available on request. We reserve the right to modify or improve the designs or specifications of our products at any time without notice.*

**WORLD HEADQUARTERS  
AND AMERICAS**

**Emerson Process Management  
Rosemount Analytical Inc.**

6565 P Davis Industrial Parkway  
Solon, OH 44139 USA  
T 440.914.1261  
Toll Free in US and Canada 800.433.6076  
F 440.914.1271  
e-mail: [gas.csc@Emerson.com](mailto:gas.csc@Emerson.com)  
[www.raihome.com](http://www.raihome.com)  
**National Response Center 800.654.7768**

**ASIA-PACIFIC**

**Emerson Process Management  
Asia Pacific Private Limited**

1 Pandan Crescent  
Singapore 128461  
Republic of Singapore  
T 65 6 777 8211  
F 65 6 777 0947  
e-mail: [analytical@ap.emersonprocess.com](mailto:analytical@ap.emersonprocess.com)

**ROSEMOUNT ANALYTICAL EUROPE**

**Emerson Process Management  
GmbH & Co. OHG**

Industriestrasse 1  
63594 Hasselroth  
Germany  
T 49 6055 884 0  
F 49 6055 884209

**EUROPE**

**Emerson Process Management  
Shared Services Limited**

Heath Place  
Bognor Regis  
West Sussex PO22 9SH  
England  
T 44 1243 863121  
F 44 1243 845354

**LATIN AMERICA**

**Emerson Process Management  
Rosemount Analytical**

11100 Brittmoores Park Road  
Houston, TX 77041 USA  
T 713.467.6000  
F 713.827.3328

**MIDDLE EAST AND AFRICA**

**Emerson Process Management**

EPM Building  
P.O. Box 17033  
Jebel Ali Free Zone  
Dubai, United Arab Emirates  
T 971 4 8835235  
F 971 4 8835312



**EMERSON™**  
Process Management